

**Human Cytokine/Chemokine
Magnetic Bead Panel III**

96 Well Plate Assay

**Cat. # HCYP3MAG-63K
HCP3MAG-63K-PX9 and
HCP3MAG-63K-PX11**

MILLIPLEX[®] MAP

HUMAN CYTOKINE / CHEMOKINE MAGNETIC BEAD PANEL III KIT 96 Well Plate Assay

#HCYP3MAG-63K
or #HCP3MAG-63K-PX9 (9-plex premixed)
or #HCP3MAG-63K-PX11 (11-plex premixed)

<u>TABLE OF CONTENTS</u>	<u>PAGE</u>
Introduction	2
Principle	3
Storage Conditions Upon Receipt	3
Reagents Supplied	5
Materials Required But Not Provided	6
Safety Precautions	6
Technical Guidelines	6
Sample Collection And Storage	7
Preparation of Reagents for Immunoassay	9
Immunoassay Procedure	12
Plate Washing	15
Equipment Settings	15
Quality Controls	17
Assay Characteristics	17
Troubleshooting Guide	19
Replacement Reagents	22
Ordering Information	23
Well Map	24

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

By purchasing this product, which contains fluorescently labeled microsphere beads authorized by Luminex Corporation ("Luminex"), you, the customer, acquire the right under Luminex's patent rights, if any, to use this product or any portion of this product, including without limitation the microsphere beads contained herein, only with Luminex's laser based fluorescent analytical test instrumentation marketed under the name of Luminex 100™ IS, 200™, HTS, FLEXMAP 3D™ MAGPIX[®] ..

INTRODUCTION

“Cytokine” is a general term used for a diverse group of soluble proteins and peptides which act as regulators under both normal and pathological conditions to modulate the functional activities of individual cells and tissues. These proteins also mediate direct interactions between cells and regulate processes taking place in the extracellular environment. Cytokines differ from hormones in that they act on a wider spectrum of target cells. Also, unlike hormones, they are not produced by specialized cells which are organized in specialized glands. The cytokine group of proteins includes lymphokines, interferons, colony stimulating factors and chemokines. Cytokine and chemokine research plays a significant role in achieving a deeper understanding of the immune system and its multi-faceted response to most antigens, as well as disease states such as inflammatory disease, allergic reactions, IBD, sepsis, and cancer.

To identify specific cytokines involved in any inflammatory or immune response, it might be necessary to screen panels of cytokines, often requiring some level of automation and/or high throughput. Magnetic Beads can make the process of automation and high throughput screening easier with features such as walk-away washing. Advantages outside automation include:

- More flexible plate and plate washer options
- Improved performance with turbid serum/plasma samples
- Assay results equivalent to non-magnetic beads
- Automated washing eliminates technical obstacles (i.e., clogging of wells that contain viscous samples) which may result during vacuum manifold/manual washing

Therefore, the **MILLIPLEX® MAP** Human Cytokine / Chemokine Panel III enables you to focus on the therapeutic potential of cytokines as well as the modulation of cytokine expression. Coupled with the Luminex xMAP® platform in a **magnetic bead** format, you receive the advantage of ideal speed and sensitivity, allowing quantitative multiplex detection of multiple analytes simultaneously, which can dramatically improve productivity.

Millipore's MILLIPLEX *MAP* Human Cytokine / Chemokine Panel III is an extension panel of Human Cytokine/Chemokine Panel, which is the most versatile system available for cytokine and chemokine research.

- Within panel III, MILLIPLEX® *MAP* offers you the ability to:
 - Select a 9-plex (for serum/plasma) or 11-plex (for cell culture) pre-mixed kit
 - Choose any combination of analytes from this panel of 11 analytes to design a custom kit that better meets your needs (Note: CXCL7/NAP-2 and CCL14a/HCC-1 can't be combined to all other cytokines when measuring serum/plasma due to different dilution needs).
- A convenient “all-in-one” box format gives you the assurance that you will have all the necessary reagents you need to run your assay.

Millipore's MILLIPLEX® Human Cytokine / Chemokine Panel III kit is to be used for the simultaneous quantification of the following 11 human cytokines and chemokines: M-CSF, CXCL9/MIG, CXCL7/NAP-2, CXCL6/GCP-2, CXCL11/I-TAC, CCL14a/HCC-1, CCL19/MIP-3 β , CCL20/MIP-3 α , XCL1/Lymphotactin, IL-11, and IL-29/IFN- λ 1. **Note: CXCL7/NAP-2 and CCL14a/HCC-1 cannot be combined to all other cytokines when measuring serum/plasma due to different dilution needs**

This kit is for research purposes only.

Please read entire protocol before use.

It is important to use same assay incubation conditions throughout your study.

PRINCIPLE

MILLIPLEX MAP is based on the Luminex® xMAP® technology — one of the fastest growing and most respected multiplex technologies offering applications throughout the life-sciences, and is capable of performing a variety of bioassays including immunoassays on the surface of fluorescent-coded magnetic beads known as MagPlex™-C microspheres.

- Luminex uses proprietary techniques to internally color-code microspheres with two fluorescent dyes. Through precise concentrations of two dyes, 100 distinctly colored bead sets can be created, each of which is coated with a specific capture antibody.
- After an analyte from a test sample is captured by the bead, a biotinylated detection antibody is introduced.
- The reaction mixture is then incubated with Streptavidin PE conjugate, the reporter molecule, to complete the reaction on the surface of each microsphere.
- The microspheres are allowed to pass rapidly through a laser, which excites the internal dyes marking the microsphere set. A second laser excites PE, the fluorescent dye on the reporter molecule.
- Finally, high-speed digital-signal processors identify each individual microsphere and quantify the result of its bioassay, based on fluorescent reporter signals.

The capability of adding multiple conjugated beads to each sample results in the ability to obtain multiple results from each sample. Open-architecture xMAP technology enables multiplexing of many types of bioassays reducing time, labor and costs over traditional methods.

STORAGE CONDITIONS UPON RECEIPT

- Recommended storage for kit components is 2 - 8 °C.
- Once the standards and controls have been reconstituted, immediately transfer contents into polypropylene vials. **DO NOT STORE RECONSTITUTED STANDARDS OR CONTROLS IN GLASS VIALS.** For long-term storage, freeze reconstituted standards and controls at $\leq -20^{\circ}\text{C}$. Avoid multiple (>2) freeze thaw cycles.
- **DO NOT FREEZE Antibody-Immobilized Beads, Detection Antibodies, and Streptavidin-Phycoerythrin.**

REAGENTS SUPPLIED

Note: Store all reagents at 2 – 8 °C

REAGENTS SUPPLIED	CATALOG NUMBER	VOLUME	QUANTITY
Human Cytokine / Chemokine Panel III Standard	MXH8063	Lyophilized	1 vial
Human Cytokine Panel III Quality Controls 1 and 2	MXH6063	Lyophilized	2 vials
Serum Matrix Note: Contains 0.08% Sodium Azide	MXHSM-3	Lyophilized	1 vial (required for serum and plasma samples only)
Set of one 96-Well Plates with 2 Sealers	-----	-----	1 plates 2 sealers
Assay Buffer	L-AB	30 mL	1 bottle
Bead Diluent (not provided with premixed panel)	LBD	3.5mL	1bottle
10X Wash Buffer Note: Contains 0.05% Proclin	L-WB	30 mL	2 bottles
Human Cytokine Panel III Detection Antibodies	MXH1063-1 or MXH1063-2	3.2 mL	1 bottle
Streptavidin-Phycoerythrin	L-SAPE6	3.2 mL	1 bottle
Mixing Bottle (not provided with premixed panel)	-----	-----	1 bottle

Human Cytokine / Chemokine Panel III Antibody-Immobilized Premixed Magnetic Beads:

Premixed 9-plex Beads	HCP3PMX9-MAG	3.5 mL	1 bottle
Premixed 11-plex Beads (tissue culture only)	HCP3PMX9-MAG, HNAP2-MAG, HHCC1-MAG	3.5 mL 90 µL 90 µL	1 bottle + 2 bead vials

Human Cytokine / Chemokine Panel III Antibody-Immobilized Magnetic Beads:

Bead/Analyte Name	Luminex Magnetic Bead Region	Customizable 11 Analytes (50X concentration, 90µL) Available Cat. #		9-Plex Premixed Beads	9-Plex Premixed Beads + 2 vials
Anti-Human M-CSF Bead	51	✓	HMCSF-MAG	✓	✓
Anti-Human CXCL9/MIG Bead	47	✓	HMIG-MAG	✓	✓
Anti-Human CXCL7/NAP2 Bead	13	✓	HNAP2-MAG		✓ Single Vial
Anti-Human CXCL6/GCP2 Bead	15	✓	HGCP2-MAG	✓	✓
Anti-Human CXCL11/I-TAC Bead	19	✓	HITAC-MAG	✓	✓
Anti-Human CCL14a/HCC-1 Bead	21	✓	HHCC1-MAG		✓ Single Vial
Anti-Human CCL19/MIP3β bead	26	✓	HMIP3B-MAG	✓	✓
Anti-Human CCL20/MIP3α Bead	28	✓	HMIP3A-MAG	✓	✓
Anti-Human XCL1/Lymphotactin Bead	30	✓	HLTCTN-MAG	✓	✓
Anti-Human IL-11 Bead	34	✓	HIL11-MAG	✓	✓
Anti-Human IL-29/IFN-λ1 Bead	36	✓	HIL29-MAG	✓	✓

MATERIALS REQUIRED BUT NOT PROVIDED

Reagents

1. Luminex Sheath Fluid (Luminex Catalogue #40-50000) or Luminex Drive Fluid (Luminex Catalogue # MPXDF-4PK)

Instrumentation / Materials

1. Adjustable Pipettes with Tips capable of delivering 25 μ L to 1000 μ L
 2. Multichannel Pipettes capable of delivering 5 μ L to 50 μ L or 25 μ L to 200 μ L
 3. Reagent Reservoirs
 4. Polypropylene Microfuge Tubes
 5. Rubber Bands
 6. Aluminum Foil
 7. Absorbent Pads
 8. Laboratory Vortex Mixer
 9. Sonicator (Branson Ultrasonic Cleaner Model #B200 or equivalent)
 10. Titer Plate Shaker (Lab-Line Instruments Model #4625 or equivalent)
 11. Luminex 200™, HTS, FLEXMAP 3D™ or MAGPIX® with xPONENT software by Luminex Corporation
 12. Automatic Plate washer for magnetic beads (Bio-Tek ELx405, Millipore catalog #40-015 or equivalent) or Hand held Magnetic Separation Block (Millipore catalog # 40-285 or equivalent)
- 5)

Note: If a plate washer or hand held magnetic separation block for magnetic beads is not available, one can use Microtiter filter plate (MX-PLATE) to run the assay with the use of Vacuum Filtration Unit (Millipore Vacuum Manifold Catalog #MSVMHTS00, or equivalent. Millipore Vacuum Pump Catalog #WP6111560 or equivalent.)

SAFETY PRECAUTIONS

- All blood components and biological materials should be handled as potentially hazardous. Follow universal precautions as established by the Centers for Disease Control and Prevention and by the Occupational Safety and Health Administration when handling and disposing of infectious agents.
- Sodium Azide or Proclin has been added to some reagents as a preservative. Although the concentrations are low, Sodium Azide and Proclin may react with lead and copper plumbing to form highly explosive metal azides. On disposal, flush with a large volume of water to prevent azide build up.

TECHNICAL GUIDELINES

To obtain reliable and reproducible results, the operator should carefully read this entire manual and fully understand all aspects of each assay step before running the assay. The following notes should be reviewed and understood before the assay is set-up.

- FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.
- Do not use beyond the expiration date on the label.
- Do not mix or substitute reagents with those from other lots or sources.

- The Antibody-Immobilized Beads are light sensitive and must be protected from light at all times. Cover the assay plate containing beads with opaque plate lid or aluminum foil during all incubation steps.
- It is important to allow all reagents to warm to room temperature (20-25°C) before use in the assay.
- Incomplete washing can adversely affect the assay outcome. All washing must be performed with the Wash Buffer provided.
- After hydration, all standards and controls must be transferred to polypropylene tubes.
- The standards prepared by serial dilution must be used within 1 hour of preparation. Discard any unused standards except the standard stock which may be stored at $\leq -20^{\circ}\text{C}$ for 1 month and at $\leq -80^{\circ}\text{C}$ for greater than one month.
- If samples fall outside the dynamic range of the assay, further dilute the samples with the appropriate diluent and repeat the assay.
- Any unused mixed Antibody-Immobilized Beads may be stored in the Bead Mix bottle at 2-8°C for up to one month.
- During the preparation of the standard curve, make certain to mix the higher concentration well before making the next dilution. Use a new tip with each dilution.
- The plate should be read immediately after the assay is finished. If, however, the plate cannot be read immediately, seal the plate, cover with aluminum foil or an opaque lid, and store the plate at 2-8°C for up to 24 hours. Prior to reading, agitate the plate on the plate shaker at room temperature for 10 minutes. Delay in reading a plate may result in decreased sensitivity for some analytes.
- The titer plate shaker should be set at a speed to provide maximum orbital mixing without splashing of liquid outside the wells. For the recommended plate shaker, this would be a setting of 5-7, which is approximately 500-800 rpm.
- Ensure that the needle probe is clean. This may be achieved by sonication and/or alcohol flushes.
- When reading the assay on Luminex 200™, adjust probe height according to the protocols recommended by Luminex to the kit solid plate using 4 alignment discs. When reading the assay on FLEXMAP 3D™, adjust probe height according to the protocols recommended by Luminex to the kit solid plate using 1 alignment disc. When reading the assay on MAGPIX, adjust probe height according to the protocols recommended by Luminex to the kit solid plate using 2 alignment disc.
- For cell culture supernatants or tissue extracts, use the culture or extraction medium as the matrix solution in blank, standard curve and control wells.
- For cell/tissue homogenate, the final cell or tissue homogenate should be prepared in a buffer that has a neutral pH, contains minimal detergents or strong denaturing detergents, and has an ionic strength close to physiological concentration. Avoid debris, lipids, and cell/tissue chunks. Centrifuge samples before use.
- Vortex all reagents well before adding to plate.

SAMPLE COLLECTION AND STORAGE

A. Preparation of Serum Samples:

- Allow the blood to clot for at least 30 minutes before centrifugation for 10 minutes at 1000xg. Remove serum and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (>2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- For all analytes **except** NAP2 and HCC-1, neat serum samples are used. However, if further dilution of neat serum is required, use the Serum Matrix as the diluent. Additional Serum Matrix can be purchased from Millipore (Millipore Catalog #MXHSM-3).
- ***When NAP2 and HCC-1 are measured separately in serum***, the serum samples should be diluted 1:100 in the Assay Buffer. Accordingly, for these analytes Serum Matrix diluted 1:100 in Assay Buffer should be used as the matrix for the standard curve and quality control wells. If serum samples require further dilution beyond 1:100, continue to use Assay Buffer as the sample diluent, and 1:100 diluted Serum Matrix as the matrix for standard curve/quality control wells.

B. Preparation of Plasma Samples:

- Plasma collection using EDTA as an anti-coagulant is recommended. Centrifuge for 10 minutes at 1000xg within 30 minutes of blood collection. Remove plasma and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (>2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- For all analytes **except** NAP2 and HCC-1, neat plasma samples are used. However, if further dilution of neat plasma is required, use the Serum Matrix as the diluent. Additional Serum Matrix can be purchased from Millipore (Millipore Catalog #MXHSM-3).
- ***When NAP2 and HCC-1 are measured separately in plasma***, the plasma samples should be diluted 1:100 in the Assay Buffer. Accordingly, for these analytes Serum Matrix diluted 1:100 in Assay Buffer should be used as the matrix for the standard curve and quality control wells. If serum samples require further dilution beyond 1:100, continue to use Assay Buffer as the sample diluent, and 1:100 diluted Serum Matrix as the matrix for standard curve/quality control wells.

C. Preparation of Tissue Culture Supernatant:

- Centrifuge the sample to remove debris and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (>2) freeze/thaw cycles.
- Tissue culture supernatant may require a dilution with an appropriate control medium prior to assay.

NOTE:

- A maximum of 25 μL per well of neat or diluted serum or plasma can be used. Tissue culture or other media may also be used.
- All samples must be stored in polypropylene tubes. **DO NOT STORE SAMPLES IN GLASS.**
- Avoid debris, lipids and cells when using samples with gross hemolysis or lipemia.
- Care must be taken when using heparin as an anticoagulant since an excess of heparin will provide falsely high values. Use no more than 10 IU heparin per mL of blood collected.

PREPARATION OF REAGENTS FOR IMMUNOASSAY

A. Preparation of Antibody-Immobilized Magnetic Beads

If premixed beads (9-plex) are used, sonicate the premixed bead bottle 30 seconds and then vortex for 1 minute before use.

To prepare 11-plex premixed beads for tissue/cell lysate and culture supernatant samples, add 70 μL of each additional bead (HNAP2-MAG and HHCC1-MAG) to the 9-plex premixed beads. Mix well before use.

For individual vials of beads, sonicate each antibody-bead vial for 30 seconds; vortex for 1 minute. Add 60 μL from each antibody bead vial to the Mixing Bottle and bring final volume to 3.0 mL with Bead Diluent. Vortex the mixed beads well. Unused portion may be stored at $2-8^{\circ}\text{C}$ for up to one month. (Note: Due to the composition of magnetic beads, you may notice a slight color in the bead solution. This does not affect the performance of the beads or the kit.)

Example 1: When using 5 cytokine antibody-immobilized beads, add 60 μL from each of the 5 bead sets to the Mixing Bottle. Then add 2.7mL Bead Diluent.

Example 2: When using 8 cytokine antibody-immobilized beads, add 60 μL from each of the 8 bead sets to the Mixing Bottle. Then add 2.52 mL Bead Diluent.

B. Preparation of Quality Controls

Before use, reconstitute Quality Control 1 and Quality Control 2 with 250 μL deionized water. Invert the vial several times to mix and vortex. Allow the vial to sit for 5-10 minutes and then transfer the controls to appropriately labeled polypropylene microfuge tubes. Unused portion may be stored at $\leq -20^{\circ}\text{C}$ for up to one month.

C. Preparation of Wash Buffer

Bring the 10X Wash Buffer to room temperature and mix to bring all salts into solution. Dilute 60 mL of 10X Wash Buffer with 540 mL deionized water. Store unused portion at 2-8°C for up to one month.

D. Preparation of Serum Matrix

This step is required for serum or plasma samples only.

Add 1.0 mL deionized water to the bottle containing lyophilized Serum Matrix. Mix well. Allow at least 10 minutes for complete reconstitution. Leftover reconstituted Serum Matrix should be stored at $\leq -20^{\circ}\text{C}$ for up to one month.

E. Preparation of Human Cytokine Panel III Standard

1.) Prior to use, reconstitute the Human Cytokine Panel III Standard with 250 μL deionized water to give Standard 6. Invert the vial several times to mix. Vortex the vial for 10 seconds. Allow the vial to sit for 5-10 minutes and then transfer the standard to an appropriately labeled polypropylene microfuge tube. The unused portion of Standard 6 may be stored at $\leq -20^{\circ}\text{C}$ for up to one month.


2.) Preparation of Working Standard (Std):

Label five polypropylene microfuge tubes Std 5, Std 4, Std 3, Std 2 and Std 1. Add 150 μL of Assay Buffer to each of the five tubes. Prepare 4-fold serial dilutions by adding 50 μL of the reconstituted Standard 6 to the Std 5 tube, mix well and transfer 50 μL of the Std 5 to the Std 4 tube, mix well and transfer 50 μL of the Std 4 to the Std 3 tube, mix well and transfer 50 μL of the Std 3 to Std 2 tube, mix well and transfer 50 μL of the Std 2 to the Std 1 tube and mix well. The Standard 0 (Background) will be Assay Buffer.

Standard	Volume of Deionized Water to Add	Volume of Standard to Add
Original (Standard 6)	250 μL	0

Standard	Volume of Assay Buffer to Add	Volume of Standard to Add
Standard 5	150 μL	50 μL of Standard 6
Standard 4	150 μL	50 μL of Standard 5
Standard 3	150 μL	50 μL of Standard 4
Standard 2	150 μL	50 μL of Standard 3
Standard 1	150 μL	50 μL of Standard 2

Preparation of Working Standard (Std):

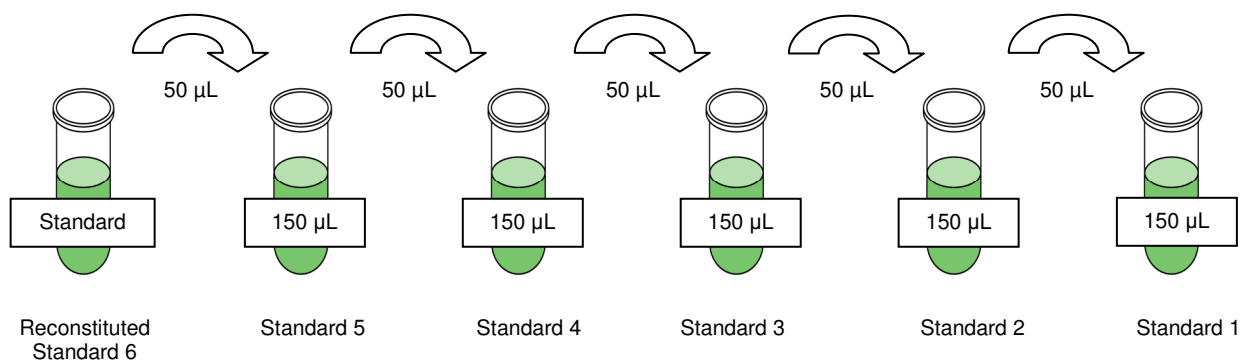

After serial dilutions, the standard tubes should have the following concentrations for the analytes, as noted below:

Standard Tube #	CXCL11/ I-TAC (pg/mL)	CXCL6/GCP-2, CCL14a/HCC-1, CCL19/MIP-3β, CCL20/MIP-3α (pg/mL)	CXCL7/NAP-2, XCL1/Lymphotoctin, IL-11 (pg/mL)	CXCL9/MIG (pg/mL)	M-CSF (pg/mL)	IL-29/ IFN-λ1 (pg/mL)
1	1.95	9.77	19.53	48.83	97.66	195.31
2	7.81	39.06	78.13	195.31	390.63	781.25
3	31.25	156.25	312.5	781.25	1,562.5	3,125
4	125	625	1,250	3,125	6,250	12,500
5	500	2,500	5,000	12,500	25,000	50,000
6	2,000	10,000	20,000	50,000	100,000	200,000

IMMUNOASSAY PROCEDURE

- Prior to beginning this assay, it is imperative to read this protocol completely and to thoroughly understand the Technical Guidelines.
- Allow all reagents to warm to room temperature (20-25°C) before use in the assay.
- Diagram the placement of Standards [Std 0 (Background), Std 1, Std 2, Std 3, Std 4, Std 5, Std 6], Controls 1 and 2, and Samples on Well Map Worksheet in a vertical configuration. (Note: Most instruments will only read the 96-well plate vertically by default.) It is recommended to run the assay in duplicate.
- If using a filter plate, set the filter plate on a plate holder at all times during reagent dispensing and incubation steps so that the bottom of the plate does not touch any surface.

1. Add 200 µL of Assay Buffer into each well of the plate. Seal and mix on a plate shaker for 10 minutes at room temperature (20-25°C).
2. Decant Wash Buffer and remove the residual amount from all wells by inverting the plate and tapping it smartly onto absorbent towels several times.
3. Add 25 µL of each Standard or Control into the appropriate wells. Assay Buffer should be used for the Std 0 (Background) wells.
4. Add 25 µL of Assay Buffer to the sample wells.
5. Add 25 µL of appropriate matrix solution to the background, standards, and control wells. When assaying neat serum or plasma, use the neat Serum Matrix provided in the kit. When using 1:100 diluted serum or plasma, use 1:100 diluted Serum Matrix for the matrix solution. When assaying tissue culture or other supernatant, use proper control culture medium as the matrix solution.
6. Add 25 µL of Sample into the appropriate wells.
7. Vortex Mixing Bottle and add 25 µL of the Mixed or Premixed Beads to each well. (Note: During addition of Beads, shake bead bottle intermittently to avoid settling.)
8. Seal the plate with a plate sealer, and wrap the plate with aluminum foil. Incubate with agitation on a plate shaker overnight at 4°C or 2 hours at room temperature (20-25°C). *An overnight incubation (16-18 hr) may improve assay sensitivity for some analytes.*

Add 200 µL Assay Buffer per well



Shake 10 min, RT

Decant

- Add 25 µL Standard or Control to appropriate wells
- Add 25 µL Assay Buffer to background and sample wells
- Add 25 µL appropriate matrix to background, standards, and control wells
- Add 25 µL Samples to sample wells
- Add 25 µL Beads to each well



Incubate overnight at 4°C or 2 hours at RT with shaking

9. Gently remove well contents and wash plate 2 times following instructions listed in the **PLATE WASHING** section.
10. Add 25 μ L of Detection Antibodies into each well. (Note: Allow the Detection Antibodies to warm to room temperature prior to addition.)
11. Seal, cover with foil and incubate with agitation on a plate shaker for 1 hour at room temperature (20-25°C). **DO NOT ASPIRATE AFTER INCUBATION.**
12. Add 25 μ L Streptavidin-Phycoerythrin to each well containing the 25 μ L of Detection Antibodies.
13. Seal, cover with foil and incubate with agitation on a plate shaker for 30 minutes at room temperature (20-25°C).
14. Gently remove well contents and wash plate 2 times following instructions listed in the **PLATE WASHING** section.
15. Add 150 μ L of Sheath Fluid (or Drive Fluid if using MAGPIX®) to all wells. Resuspend the beads on a plate shaker for 5 minutes.



Remove well contents and wash 2X with 200 μ L Wash Buffer

Add 25 μ L Detection Antibodies per well



Incubate 1 hour at RT

Do Not Aspirate

Add 25 μ L Streptavidin-Phycoerythrin per well

Incubate for 30 minutes at RT



Remove well contents and wash 2X with 200 μ L Wash Buffer

Add 150 μ L Sheath Fluid or Drive Fluid per well

16. Run plate on Luminex 200™, HTS, FLEXMAP 3D™ or MAGPIX® with xPONENT software.
17. Save and analyze the Median Fluorescent Intensity (MFI) data using a 5-parameter logistic or spline curve-fitting method for calculating cytokine/chemokines concentrations in samples. (Note: For diluted samples, multiply the calculated concentration by the dilution factor.)

Read on Luminex (100 µL, 50 beads per bead set)
--

PLATE WASHING

1.) Solid Plate

If using a solid plate, use either a hand-held magnet or magnetic plate washer.

A.) For hand-held magnet, rest plate on magnet for 60 seconds to allow complete settling of magnetic beads. Remove well contents by gently decanting the plate in an appropriate waste receptacle and gently tapping on absorbent pads to remove residual liquid. Wash plate with 200 µL of Wash Buffer by removing plate from magnet, adding Wash Buffer, shaking for 30 seconds, reattaching to magnet, letting beads settle for 60 seconds and removing well contents as previously described after each wash. Repeat wash steps as recommended in Assay Procedure.

B.) For magnetic plate washer, let plate “soak” on magnet for 60 seconds to allow complete settling of the magnetic beads. Remove well contents by aspiration. Wash plate with 200 µL/well of Wash Buffer, letting beads “soak” for 60 seconds and removing Wash Buffer by aspiration after each wash. Repeat wash steps as recommended in Assay Procedure. **Note:** If using the recommended plate washer for magnetic beads (Bio-Tek ELx405) follow the appropriate equipment settings outlined in **EQUIPMENT SETTINGS**.

2.) Filter Plate (Millipore Cat# MX-PLATE)

If using a filter plate, use a vacuum filtration manifold to remove well contents. Wash plate 200 µL/well of Wash Buffer, removing Wash Buffer by vacuum filtration after each wash. Repeat wash steps as recommended in the Assay Procedure.

EQUIPMENT SETTINGS

Bio-Tek ELx405:

The general recommended wash protocol (Link Protocol) is as follows:

Soak Program: Wash Program:

Soak → Aspirate→Dispense→Soak→Aspirate→Dispense→Soak→Aspirate

1.) Soak program:

1. Soak duration: 60 sec
2. Shake before soak?: NO

2.) Wash program:

Method:

1. Number of cycles: 2
2. soak/shake: YES
3. Soak duration: 60 sec
4. Shake before soak: NO
5. Prime after soak: NO

Dispense:

1. Dispense volume: 200 µL/well
2. Dispense flow rate: 5
3. Dispense height: 130 (16.51 mm)
4. Horizontal disp pos: 00 (0 mm)
5. Bottom Wash first?: NO
6. Prime before start?: NO

Aspiration:

1. Aspirate height: 35 (4.445 mm)
2. Horizontal Asp Pos: 30 (1.372 mm)
3. Aspiration rate: 06 (15.0 mm/sec)
4. Aspiration delay: 0
5. Crosswise Aspir: NO
6. Final Aspir: YES
7. Final Aspir delay: 0 (0 msec)

- 3.) Link program: (**Note:** this is the program to use during actual plate washing).
Link together the Soak and Wash programs outlined above.

Note: After the final aspiration, there will be approximately 25 µl of residual Wash Buffer in each well. This is expected when using the BioTek Plate washer and this volume does not need to be aspirated from the plate.

If using an automatic plate washer other than BioTek ELx405, please refer to the manufacturers's recommendations for programming instructions.

EQUIPMENT SETTINGS (continued)

These specifications are for the Luminex 200™, Luminex HTS, Luminex FLEXMAP 3D™ and Luminex MAGPIX® with xPonent software. Luminex instruments with other software (e.g. MasterPlex, StarStation, LiquiChip, Bio-Plex, LABScan100) would need to follow instrument instructions for gate settings and additional specifications from the vendors for reading Luminex Magnetic Beads.

For magnetic bead assays, the Luminex 200™ and HTS instruments must be calibrated with the xPonent 3.1 compatible Calibration Kit (Millipore Cat.# 40-275) and performance verified with the Performance Verification Kit (Millipore Cat. # 40-276). The Luminex FLEXMap 3D™ instrument must be calibrated with the FLEXMAP 3D™ Calibrator Kit (Millipore cat#40-028) and performance verified with the FLEXMAP 3D™ Performance Verification Kit (Millipore cat#40-029). The Luminex MAGPIX® instrument must be calibrated with the MAGPIX® Calibration Kit (Millipore cat# 40-049 and performance verified with the MAGPIX® Performance Verification Kit (Millipore cat# 40-050).

NOTE: These assays cannot be run on Luminex 100™ instruments or any instruments using Luminex IS 2.3 or Luminex 1.7 software.

The Luminex probe height must be adjusted to the plate provided in the kit. Please use Cat.# MAG-PLATE, if additional plates are required for this purpose.

Events:	50, per bead			
Sample Size:	100 µL			
Gate Settings:	8,000 to 15,000			
Reporter Gain	Default (low PMT)			
Time Out	200 seconds			
Bead Set:	9-Plex Premix Beads		Customizable 11-Plex Beads	
	M-CSF	51	M-CSF	51
	CXCL9/MIG	47	CXCL9/MIG	47
	CXCL6/GCP-2	15	CXCL7/NAP-2	13
	CXCL11/I-TAC	19	CXCL6/GCP-2	15
	CCL19/MIP-3β	26	CXCL11/I-TAC	19
	CCL20/MIP-3α	28	CCL14a/HCC-1	21
	XCL1/Lymphotactin	30	CCL19/MIP-3β	26
	IL-11	34	CCL20/MIP-3α	28
	IL-29/IFN-λ1	36	XCL1/Lymphotactin	30
			IL-11	34
			IL-29/IFN-λ1	36

QUALITY CONTROLS

The ranges for each analyte in Quality Control 1 and 2 are provided on the card insert or can be located at the Millipore website www.millipore.com/techlibrary/index.do using the catalog number as the keyword.

ASSAY CHARACTERISTICS

Assay Sensitivities (minimum detectable concentrations, pg/mL)

MinDC: Minimum Detectable Concentration is calculated by the StatLIA® Immunoassay Analysis Software from Brendan Technologies. It measures the true limits of detection for an assay by mathematically determining what the empirical MinDC would be if an infinite number of standard concentrations were run for the assay under the same conditions.

Cytokine	Overnight Protocol (N=8)
	MinDC+2SD (pg/mL)
M-CSF	563.6
CXCL9/MIG	19.2
CXCL7/NAP2	11.2
CXCL6/GCP2	2.5
CXCL11/I-TAC	1.7
CCL14a/HCC-1	2.0
CCL19/MIP3 β	3.1
CCL20/MIP3 α	2.0
XCL1/Lymphotactin	26.5
IL-11	14.5
IL-29/IFN- λ 1	95.8

Precision

Intra-assay precision is generated from the mean of the % CV's from 8 reportable results across two different concentrations of cytokines in an overnight or 1-day assay. Inter-assay precision is generated from the mean of the % CV's across two different concentrations of cytokines across 6 different overnight assays.

Cytokine	Overnight Protocol	
	Intra-Assay %CV	Inter-Assay %CV
M-CSF	9.1	24.4
CXCL9/MIG	1.8	23.0
CXCL7/NAP2	3.3	6.0
CXCL6/GCP2	2.2	12.4
CXCL11/I-TAC	2.7	14.9
CCL14a/HCC-1	2.1	3.7
CCL19/MIP3 β	1.9	13.3
CCL20/MIP3 α	2.1	11.6
XCL1/Lymphotactin	1.7	8.4
IL-11	2.4	11.5
IL-29/IFN- λ 1	2.6	9.8

Accuracy

Spike Recovery: The data represent mean percent recovery of spiked standards ranging from 31 to 46,146 pg/mL in serum matrix samples (N=6).

Cytokine	Overnight Protocol
	Recovery
M-CSF	92.3
CXCL9/MIG	100.4
CXCL7/NAP2	99.0
CXCL6/GCP2	103.8
CXCL11/I-TAC	101.9
CCL14a/HCC-1	105.9
CCL19/MIP3 β	98.9
CCL20/MIP3 α	103.4
XCL1/Lymphotactin	98.5
IL-11	95.6
IL-29/IFN- λ 1	104.6

Cross-Reactivity

There was no or negligible cross-reactivity between the antibodies and any of the other analytes in this panel.

TROUBLESHOOTING GUIDE

Problem	Probable Cause	Solution
Insufficient Bead Count	Plate Washer aspirate height set too low	Adjust aspiration height according to manufacturers instructions.
	Bead mix prepared inappropriately	Sonicate bead vials and vortex just prior to adding to bead mix bottle according to protocol. Agitate bead mix intermittently in reservoir while pipetting this into the plate.
	Samples cause interference due to particulate matter or viscosity	See above. Also sample probe may need to be cleaned with Alcohol flush, Back flush and washes; or if needed probe should be removed and sonicated.
	Probe height not adjusted correctly	When reading the assay on Luminex 200™, adjust probe height according to the protocols recommended by Luminex to the kit solid plate using 4 alignment discs. When reading the assay on FLEXMAP 3D™, adjust probe height according to the protocols recommended by Luminex to the kit solid plate using 1 alignment disc. When reading the assay on MAGPIX, adjust probe height according to the protocols recommended by Luminex to the kit solid plate using 2 alignment disc.
Background is too high	Background wells were contaminated	Avoid cross-well contamination by using sealer appropriately, and pipeting with Multichannel pipets without touching reagent in plate.
	Matrix used has endogenous analyte or interference	Check matrix ingredients for cross reacting components (e.g. interleukin modified tissue culture medium).
	Insufficient washes	Increase number of washes.
Beads not in region or gate	Luminex not calibrated correctly or recently	Calibrate Luminex based on Instrument Manufacturer's instructions, at least once a week or if temperature has changed by >3°C.
	Gate Settings not adjusted correctly	Some Luminex instruments (e.g. Bioplex) require different gate settings than those described in the Kit protocol. Use Instrument default settings.
	Wrong bead regions in protocol template	Check kit protocol for correct bead regions or analyte selection.
	Incorrect sample type used	Samples containing organic solvents or if highly viscous should be diluted or dialyzed as required.
	Instrument not washed or primed	Prime the Luminex 4 times to rid of air bubbles, wash 4 times with sheath fluid or water if there is any remnant alcohol or sanitizing liquid.
	Beads were exposed to	Keep plate and bead mix covered with dark

	light	lid or aluminum foil during all incubation steps.
Signal for whole plate is same as background	Incorrect or no Detection Antibody was added Streptavidin-Phycoerythrin was not added	Add appropriate Detection Antibody and continue. Add Streptavidin-Phycoerythrin according to protocol. If Detection Antibody has already been removed, sensitivity may be low.
Low signal for standard curve	Detection Antibody may have been removed prior to adding Streptavidin Phycoerythrin Incubations done at inappropriate temperatures, timings or agitation	May need to repeat assay if desired sensitivity not achieved. Assay conditions need to be checked.
Signals too high, standard curves are saturated	Calibration target value set too high Plate incubation was too long with standard curve and samples	With some Luminex Instrument (e.g. Bio-plex) Default target setting for RP1 calibrator is set at High PMT. Use low target value for calibration and reanalyze plate. Use shorter incubation time.
Sample readings are out of range	Samples contain no or below detectable levels of analyte Samples contain analyte concentrations higher than highest standard point. Standard curve was saturated at higher end of curve.	If below detectable levels, it may be possible to use higher sample volume. Check with tech support for appropriate protocol modifications. Samples may require dilution and reanalysis for just that particular analyte. See above.
High Variation in samples and/or standards	Multichannel pipet may not be calibrated Plate washing was not uniform Samples may have high particulate matter or other interfering substances Plate agitation was insufficient Cross well contamination	Calibrate pipets. Confirm all reagents are removed completely in all wash steps. See above. Plate should be agitated during all incubation steps using a vertical plate shaker at a speed where beads are in constant motion without causing splashing. Check when reusing plate sealer that no reagent has touched sealer. Care should be taken when using same pipet tips that are used for reagent additions and that pipet tip does not touch reagent in plate.
FOR FILTER PLATES ONLY		
Filter plate will not vacuum	Vacuum pressure is insufficient Samples have insoluble particles High lipid concentration	Increase vacuum pressure such that 0.2mL buffer can be suctioned in 3-5 seconds. Centrifuge samples just prior to assay setup and use supernatant. After centrifugation, remove lipid layer and

		use supernatant.
Plate leaked	<p>Vacuum Pressure too high</p> <p>Plate set directly on table or absorbent towels during incubations or reagent additions</p> <p>Insufficient blotting of filter plate bottom causing wicking</p> <p>Pipette touching plate filter during additions</p> <p>Probe height not adjusted correctly</p> <p>Sample too viscous</p>	<p>Adjust vacuum pressure such that 0.2mL buffer can be suctioned in 3-5 seconds. May need to transfer contents to a new (blocked) plate and continue.</p> <p>Set plate on plate holder or raised edge so bottom of filter is not touching any surface.</p> <p>Blot the bottom of the filter plate well with absorbent towels after each wash step.</p> <p>Pipette to the side of plate.</p> <p>Adjust probe to 3 alignment discs in well H6.</p> <p>May need to dilute sample.</p>

REPLACEMENT REAGENTS**Catalog #**

Human Cytokine Panel III Standard	MXH8063
Human Cytokine Panel III Quality Controls	MXH6063
Serum Matrix	MXHSM-3
Human Cytokine Panel III Detection Antibodies	MXH1063-1
	MXH1063-2
Streptavidin-Phycoerythrin	L-SAPE6
Assay Buffer	L-AB
Bead Diluent	LBD
96-Well Plates with Sealers	MAG-PLATE
10X Wash Buffer	L-WB

Antibody-Immobilized Magnetic Beads

<u>Cytokine</u>	<u>Bead #</u>	<u>Cat. #</u>
M-CSF	51	HMCSF-MAG
CXCL9/MIG	47	HMIG-MAG
CXCL7/NAP-2	13	HNAP2-MAG
CXCL6/GCP-2	15	HGCP2-MAG
CXCL11/I-TAC	19	HITAC-MAG
CCL14a/HCC-1	21	HHCC1-MAG
CCL19/MIP-3 β	26	HMIP3B-MAG
CCL20/MIP-3 α	28	HMIP3A-MAG
XCL1/Lymphotoxin	30	HLTCTN-MAG
IL-11	34	HIL11-MAG
IL-29/IFN- λ 1	36	HIL29-MAG
Premixed 9-plex Beads		HCP3PMX9-MAG
Premixed 11-plex Beads		HCP3PMX9-MAG + HNAP2-MAG and HHCC1-MAG

ORDERING INFORMATION

To place an order:

To assure the clarity of your custom cytokine kit order, please FAX the following information to our customer service department:

- Your name, telephone and/or fax number
- Customer account number
- Shipping and billing address
- Purchase order number
- Catalog number and description of product
- Quantity of kits
- Selection of MILLIPLEX[®] Cytokine Analytes/Serum Matrix Requirements

FAX: (636) 441-8050

Toll-Free US: (800) MILLIPORE

Mail Orders: Millipore Corp.
6 Research Park Drive
St. Charles, Missouri 63304 U.S.A.

For International Customers:

To best serve our international customers in placing an order or obtaining additional information about MILLIPLEX[®] products, please contact your multiplex specialist or sales representative or email our European Customer Service at customerserviceEU@Millipore.com.

Conditions of Sale

All products are for research use only. They are not intended for use in clinical diagnosis or for administration to humans or animals. All products are intended for *in vitro* use only.

Material Safety Data Sheets (MSDS)

Material Safety Data Sheets for Millipore products may be ordered by fax or phone or through our website at www.millipore.com/techlibrary/index.do

WELL MAP

	1	2	3	4	5	6	7	8	9	10	11	12
A	Standard 0 (Background)	Standard 4	QC-2 Control									
B	Standard 0 (Background)	Standard 4	QC-2 Control									
C	Standard 1	Standard 5	Sample 1									
D	Standard 1	Standard 5	Sample 1									
E	Standard 2	Standard 6	Sample 2									
F	Standard 2	Standard 6	Sample 2									
G	Standard 3	QC-1 Control	Etc.									
H	Standard 3	QC-1 Control										