

MILLIPLEX[®] MAP

Human Immunoglobulin Isotyping Kit 96 Well Plate Assay

#HGAM-301

| <u>TABLE OF CONTENTS</u> | <u>PAGE</u> |
|---|--------------------|
| Introduction | 2 |
| Principle | 2 |
| Storage Conditions Upon Receipt | 3 |
| Reagents Supplied | 3 |
| Materials Required But Not Provided | 4 |
| Safety Precautions | 4 |
| Technical Guidelines | 4 |
| Sample Collection And Storage | 6 |
| Preparation of Reagents for Immunoassay | 7 |
| Immunoassay Procedure | 9 |
| Equipment Settings | 10 |
| Quality Controls | 10 |
| Assay Characteristics | 11 |
| Troubleshooting Guide | 13 |
| Replacement Reagents | 15 |
| Ordering Information | 15 |
| Well Map | 16 |

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

By purchasing this product, which contains fluorescently labeled microsphere beads authorized by Luminex Corporation ("Luminex"), you, the customer, acquire the right under Luminex's patent rights, if any, to use this product or any portion of this product, including without limitation the microsphere beads contained herein, only with Luminex's laser based fluorescent analytical test instrumentation marketed under the name of Luminex 100™ IS, 200™, HTS.

INTRODUCTION

Produced by plasma cells and lymphocytes, immunoglobulins (antibodies) are critically involved in immune response, attaching to antigens and playing a role in their destruction.

Immunoglobulins (Ig) can be classified by isotype, classes that differ in function and antigen response due to structure variability. Five major isotypes have been identified in placental mammals: IgM, IgG, IgA, IgE and IgD (B-cell receptor) – all found in normal individuals. Immunoglobulin-deficiency disorders, such as autoimmune disease, some GI conditions and malignancies, are characterized by specific isotype deficiencies or varying concentrations of one or more isotypes. Disease states can range from the absence of one isotype class or subclass to a total deficiency of immunoglobulin classes. In addition, isotyping applications include analyzing hybridomas during antibody development.

Millipore recognizes the need to provide you with the ability to quantitate immunoglobulin classes and subclasses simultaneously. Therefore, we are proud to announce that the former Beadlyte Human Isotyping Kits have been re-launched in the MILLIPLEX MAP optimized format. In addition, our MILLIPLEX MAP Human Isotyping Kit has been designed to enable you to measure accurately human IgG subclasses (1, 2, 3, and 4), IgM, and IgA – all in one well. The xMAP multiplex technology is ideal for measuring levels of these isotypes, which not only decreases the number of assays as well as the amount of sample required, but also greatly reduces the possible inaccuracies that result from performing multiple assays.

This kit is for research purposes only.

Please read entire protocol before use.

It is important to use same assay incubation conditions throughout your study.

PRINCIPLE

MILLIPLEX® MAP is based on the Luminex® xMAP® technology — one of the fastest growing and most respected multiplex technologies offering applications throughout the life sciences and capable of performing a variety of bioassays including immunoassays on the surface of fluorescent-coded beads known as microspheres.

- Luminex® uses proprietary techniques to internally color-code microspheres with two fluorescent dyes. Through precise concentrations of these dyes, 100 distinctly colored bead sets can be created, each of which is coated with a specific capture antibody.
- After an analyte from a test sample is captured by the bead, a detection antibody conjugated to PE, the reported molecule, is introduced.
- The microspheres are allowed to pass rapidly through a laser which excites the internal dyes marking the microsphere set. A second laser excites PE, the fluorescent dye on the reporter molecule.
- Finally, high-speed digital-signal processors identify each individual microsphere and quantify the result of its bioassay based on fluorescent reporter signals.
- The capability of adding multiple conjugated beads to each sample results in the ability to obtain multiple results from each sample. Open-architecture xMAP® technology enables multiplexing of many types of bioassays reducing time, labor and costs over traditional methods.

STORAGE CONDITIONS UPON RECEIPT

- Recommended storage for kit components is 2 - 8 °C.
- Once the standards and controls have been reconstituted, immediately transfer contents into polypropylene vials. **DO NOT STORE RECONSTITUTED STANDARDS OR CONTROLS IN GLASS VIALS.** For long-term storage, freeze reconstituted standards and controls at ≤ -20 °C. Avoid multiple (>2) freeze/thaw cycles.
- **DO NOT FREEZE Antibody-Immobilized Beads or PE Antibodies.**

REAGENTS SUPPLIED

Note: Store all reagents at 2 – 8 °C

| REAGENTS SUPPLIED | CATALOG NUMBER | VOLUME | QUANTITY |
|--|----------------|---------|-----------|
| MILLIPLEX [®] MAP Anti-Human Multi-Ig Beads, 1X | HGAM-PMX6 | 3.5 mL | 1 bottle |
| MILLIPLEX [®] MAP Anti-Human κ and λ Light Chain, PE | HGAM-1301 | 50 µL | 1 tube |
| MILLIPLEX [®] MAP Human Multi-Immunoglobulin Standard | HGAM-8301 | 0.5 mL | 1 vial |
| MILLIPLEX [®] MAP Human Immunoglobulin Positive Control | PC-301 | 0.25 mL | 1 vial |
| MILLIPLEX [®] MAP Assay Buffer | L-AB | 30 mL | 2 bottles |
| Set of one 96-Well Filter Plate with 2 Sealers | MX-PLATE | ----- | 1 plate |

| Ig | IgG1 | IgG2 | IgG3 | IgG4 | IgA | IgM |
|--------|------|------|------|------|-----|-----|
| Bead # | 20 | 35 | 32 | 34 | 51 | 19 |

MATERIALS REQUIRED BUT NOT PROVIDED

Reagents

1. Luminex Sheath Fluid (Luminex Catalogue #40-50000)

Instrumentation / Materials

1. Adjustable Pipettes with Tips capable of delivering 25 μ L to 1000 μ L
2. Multichannel Pipettes capable of delivering 5 μ L to 50 μ L or 25 μ L to 200 μ L
3. Reagent Reservoirs
4. Polypropylene Microfuge Tubes
5. Rubber Bands
6. Absorbent Pads
7. Laboratory Vortex Mixer
8. Sonicator
9. Titer Plate Shaker
10. Vacuum Filtration Unit (Millipore Vacuum Manifold Catalog #MSVMHTS00 or equivalent with Millipore Vacuum Pump Catalog #WP6111560 or equivalent)
11. Luminex 100™ IS, 200™, or HTS by Luminex Corporation
12. Plate Stand (Millipore Catalog # MX-STAND)

SAFETY PRECAUTIONS

- All blood components and biological materials should be handled as potentially hazardous. Follow universal precautions as established by the Centers for Disease Control and Prevention and by the Occupational Safety and Health Administration when handling and disposing of infectious agents.
- Sodium azide or Proclin has been added to some reagents as a preservative. Although the concentrations are low, sodium azide and Proclin may react with lead and copper plumbing to form highly explosive metal azides. On disposal, flush with a large volume of water to prevent azide build up.

TECHNICAL GUIDELINES

To obtain reliable and reproducible results, the operator should carefully read this entire manual and fully understand all aspects of each assay step before running the assay. The following notes should be reviewed and understood before the assay is set up.

- FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.
- Do not use beyond the expiration date on the label.
- Do not mix or substitute reagents with those from other lots or sources.
- The Antibody-Immobilized Beads are light sensitive and must be protected from light at all times. Cover the assay plate containing beads with opaque plate lid or aluminum foil during all incubation steps.

- It is important to allow all reagents to warm to room temperature (20-25°C) before use in the assay.
- The bottom of the Microtiter Filter Plate should not be in direct contact with any surface during assay set-up or incubation times. The plate can be set on a plate stand or on the non-flat side of the plate cover or any other plate holder to raise the plate from the surface. A plate stand can be purchased separately from Millipore (Millipore Catalog #MX-STAND).
- Incomplete washing can adversely affect the assay outcome. All washing must be performed with the Assay Buffer provided.
- After the wash steps, keep the bottom of the Microtiter Filter Plate clean by blotting on paper towels or absorbent pads to prevent any leakage due to capillary action.
- Keep the vacuum suction on the plate as low as possible. It is recommended to have a vacuum setting that will remove 200 μ L of buffer in ≥ 5 seconds (equivalent to < 100 mmHg).
- The Standards prepared by serial dilution must be used within 1 hour of preparation. Discard any unused standards except the standard stock which may be transferred to polypropylene tubes and stored at $\leq -20^{\circ}\text{C}$ for 1 month and at $\leq -80^{\circ}\text{C}$ for greater than one month.
- If samples fall above the dynamic range of the assay, further dilute the samples with the appropriate diluent and repeat the assay.
- During the preparation of the standard curve, make certain to mix the higher concentration well before making the next dilution. Use a new tip with each dilution.
- The plate should be read immediately after the assay is finished.
- The titer plate shaker should be set at a speed to provide maximum orbital mixing without splashing of liquid outside the wells. For the recommended plate shaker, this would be a setting of 5-7 which is approximately 500-800 rpm.
- Ensure that the Luminex needle probe is clean. This may be achieved by sonication and/or alcohol flushes. Adjust probe height according to the protocols recommended by Luminex to the kit filter plate using 3 alignment discs prior to reading an assay.
- For cell culture supernatants, use the culture medium as the diluent in background, standard curve, and control wells. In assays using serum samples, all samples, standards, and controls should be diluted in Assay Buffer. In all cases, use Assay Buffer for wash and resuspension steps.
- Vortex all reagents well before adding to plate.

SAMPLE COLLECTION AND STORAGE

A. Preparation of Serum Samples:

- Allow the blood to clot for at least 30 minutes before centrifugation for 10 minutes at 1000xg. Remove serum and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (>2) freeze/thaw cycles.
- When using frozen samples, it is recommended to thaw the samples completely, mix well by vortexing and centrifuge prior to use in the assay to remove particulates.
- Serum samples should be diluted 1:16,000 in the Assay Buffer and a standard curve diluted in Assay Buffer should be used.
- To achieve a 1:16,000 dilution, dilute 5 μL of sample into 795 μL of ultrapure water (1:160). Immediately dilute 5 μL of the 1:160 dilution into 495 μL of Assay Buffer (1:100) dilution.

B. Preparation of Tissue Culture Supernatant:

- Centrifuge the sample to remove debris and assay immediately or aliquot and store samples at $\leq -20^{\circ}\text{C}$.
- Avoid multiple (>2) freeze/thaw cycles.
- Dilute the sample to approximately 1 $\mu\text{g/mL}$ Ig in Assay Buffer. [Cell culture supernatants samples approximately (1:5); bioreactor supernatants (1:100)].
Note: Cell culture supernatant concentrations are cell-line dependent and range from 5-50 $\mu\text{g/mL}$. Bioreactor supernatants may be as concentrated as 1 mg/mL .

NOTE:

- A maximum of 50 μL per well of diluted serum or supernatant can be used.
- All samples must be stored in polypropylene tubes. **DO NOT STORE SAMPLES IN GLASS.**
- Avoid debris, lipids and cells when using samples with gross hemolysis or lipemia.
- Care must be taken when using heparin as an anticoagulant since an excess of heparin will provide falsely high values. Use no more than 10 IU heparin per mL of blood collected.

PREPARATION OF REAGENTS FOR IMMUNOASSAY

A. Preparation of Antibody-Immobilized Beads

Sonicate the pre-mixed bead bottle 30 seconds and then vortex for 1 minute before use.

B. Preparation of Standards

Resuspend MILLIPLEX MAP Human Multi-Immunoglobulin (IgG1, IgG2, IgG3, IgG4, IgA, and IgM) Standard (Catalog # HGAM-8301) in 0.5 mL deionized water. Vortex at high speed for 15 seconds. Place on ice for 15 minutes. This is Standard 7. Note: Standards are of kappa light chain isotype and therefore will react only with anti-Human Kappa-PE detection reagent.


C. Preparation of Working Standards (Std):

Label six polypropylene microfuge tubes Std 6, Std 5, Std 4, Std 3, Std 2 and Std 1. Add 200 μ L of Assay Buffer to each of the six tubes. Prepare 3-fold serial dilutions by adding 100 μ L of the reconstituted Standard 7 to the Std 6 tube, mix well and transfer 100 μ L of the Std 6 to the Std 5 tube, mix well and transfer 100 μ L of the Std 5 to the Std 4 tube, mix well and transfer 100 μ L of the Std 4 to Std 3 tube, mix well and transfer 100 μ L of the Std 3 to the Std 2 tube and mix well and transfer 100 μ L of the Std 2 to the Std 1 tube and mix well. The Standard 0 (Background) will be Assay Buffer.

| Standard | Volume of Water to Add | Volume of Standard to Add |
|-----------------------|------------------------|---------------------------|
| Original (Standard 7) | 500 μ L | 0 |

| Standard | Volume of Assay Buffer to Add | Volume of Standard to Add |
|------------|-------------------------------|---------------------------|
| Standard 6 | 200 μ L | 100 μ L of Standard 7 |
| Standard 5 | 200 μ L | 100 μ L of Standard 6 |
| Standard 4 | 200 μ L | 100 μ L of Standard 5 |
| Standard 3 | 200 μ L | 100 μ L of Standard 4 |
| Standard 2 | 200 μ L | 100 μ L of Standard 3 |
| Standard 1 | 200 μ L | 100 μ L of Standard 2 |

Preparation of Working Standards:

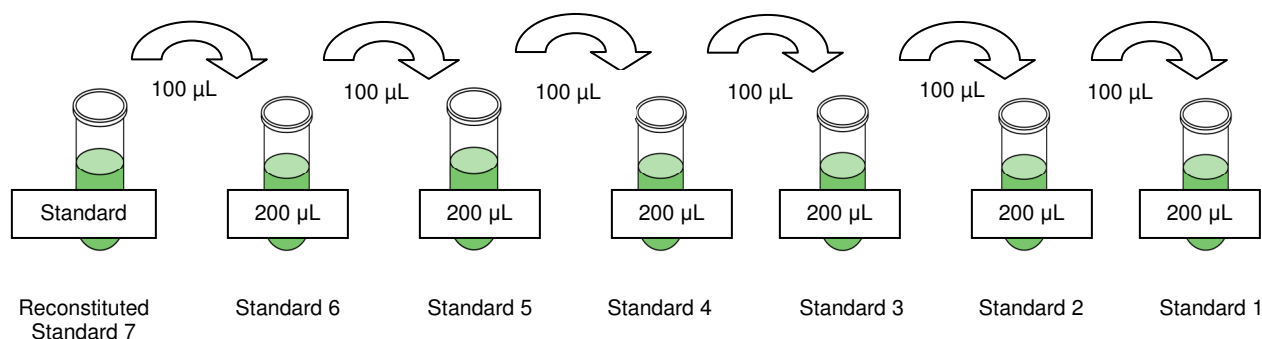

After serial dilutions, the standard tubes should have the following concentrations for the isotypes, as noted below:

| Standard Tube # | IgG1 (ng/mL) | IgG2 (ng/mL) | IgG3 (ng/mL) | IgG4 (ng/mL) | IgA (ng/mL) | IgM (ng/mL) |
|-----------------|-----------------|-----------------|-----------------|-----------------|----------------|----------------|
| 1 | 14 | 41 | 0.2 | 0.4 | 2.1 | 3.4 |
| 2 | 41 | 124 | 0.6 | 1.2 | 6.2 | 10.3 |
| 3 | 124 | 370 | 1.9 | 3.7 | 18.5 | 30.9 |
| 4 | 370 | 1111 | 5.6 | 11.1 | 55.6 | 92.6 |
| 5 | 1111 | 3333 | 16.7 | 33.3 | 166.7 | 278 |
| 6 | 3333 | 10000 | 50 | 100 | 500 | 833 |
| 7 | 10000 | 30000 | 150 | 300 | 1500 | 2500 |

D. Preparation of Positive Control

Rususpend MILLIPLEX MAP Human Multi-Ig Positive Control (Catalog # PC-301) in 0.25 mL deionized water (or cell culture medium if running with cell culture supernatants). Vortex at high speed for 15 seconds. Place on ice for 15 minutes.

E. Preparation of Human κ and λ Light Chain, PE

To prepare 100X detection reagent, dilute anti-Human Kappa and Lambda-PE to working solution (1:100) with Assay Buffer (for a full plate, use 25 µL of the 100X anti-Human kappa-PE in 2.475 mL Assay Buffer).

IMMUNOASSAY PROCEDURE

- Prior to beginning this assay, it is imperative to read this protocol completely and to thoroughly understand the Technical Guidelines.
 - Allow all reagents to warm to room temperature (20-25°C) before use in the assay.
 - Diagram the placement of Standards [0 (Background) through 7], Positive Control, and Samples on Well Map Worksheet in a vertical configuration. (Note: Most instruments will only read the 96-well plate vertically by default.) It is recommended to run the assay in duplicate.
 - Set the filter plate on a plate holder at all times during reagent dispensing and incubation steps so that the bottom of the plate does not touch any surface.
1. Pre-wet filter plate by pipetting 25 μ L of Assay Buffer into each well of the Microtiter Filter Plate. Seal and mix on a plate shaker for 10 minutes at room temperature (20-25 °C). Remove Assay Buffer by vacuum. (**NOTE: DO NOT INVERT PLATE.**) Blot excess Assay Buffer from the bottom of the plate with an absorbent pad or paper towels.
 2. Add 50 μ L of control, standard, or diluted sample to each well.
 3. Vortex the MILLIPLEX MAP Anti-Human Multi-Immunoglobulin Beads at medium speed for 15 seconds, and then sonicate for 15 seconds using a sonication bath. Add 25 μ L of bead solution to each well.
 4. Cover with opaque plate cover and incubate 1 hour with agitation on plate shaker at room temperature.
 5. Remove fluid by vacuum. Wash plate 2 times with 100 μ L of Assay Buffer. Remove Assay Buffer by vacuum filtration between each wash. Blot bottom of plate on paper towel. **Do not over-dry.**
 6. Add 25 μ L per well of diluted Anti-Human κ and λ light Chain, PE.
 7. Cover with opaque plate cover and incubate 1 hour with agitation on plate shaker at room temperature.
 8. Apply vacuum manifold to bottom of the filter plate to remove the liquid and resuspend in 150 μ L of Sheath Fluid.
 9. Proceed to reading results on an appropriate Luminex[®] instrument.

Add 25 μ L Assay Buffer per well



Shake 10 min, RT
Vacuum

- Add 50 μ L Standard or Control to appropriate wells
- Add 50 μ L diluted samples to sample wells
- Add 25 μ L Beads to each well



Incubate 1 hour at RT
with shaking in the dark

Vacuum and wash 2X
with 100 μ L Assay
Buffer

Add 25 μ L κ and λ light chain
reporter solution per well



Incubate 1 hour at
RT with shaking in
the dark

Vacuum plate and add 150 μ L
Sheath Fluid per well. Read
results using an appropriate
Luminex[®] instrument.

EQUIPMENT SETTINGS

These specifications are for the Luminex₁₀₀ v.1.7 or Luminex100IS v2.1/2.2, Luminex₂₀₀ v2.3, xPONENT, and Luminex HTS. Luminex instruments with other software (e.g. MasterPlex, StarStation, LiquiChip, Bio-Plex, LABScan100) would need to follow instrument instructions for gate settings and additional specifications from the vendors.

| | |
|---------------|-------------------|
| Events | 50 per bead |
| Sample Size | 100 µL |
| Gate Settings | 8,000 to 15,000 |
| Reporter Gain | Default (Low PMT) |
| Time Out | 60 seconds |
| Bead Set | Bead # |
| IgG1 | 20 |
| IgG2 | 35 |
| IgG3 | 32 |
| IgG4 | 34 |
| IgA | 51 |
| IgM | 19 |

QUALITY CONTROLS

The ranges for each analyte in the Human Multi-Ig Positive Control are provided on the card insert or can be located at the MILLIPORE website

www.millipore.com/techlibrary/index.do using the catalog number as the keyword.

ASSAY CHARACTERISTICS

Assay Sensitivities (minimum detectable concentrations, ng/mL)

MinDC: Minimum Detectable Concentration is calculated using Milliplex Analyst Software from Millipore. It measures the true limits of detection for an assay by mathematically determining what the empirical MinDC would be if an infinite number of standard concentrations were run for the assay under the same conditions.

| Analyte | MinDC |
|----------------|--------------|
| IgM | 0.5 |
| IgG1 | 13.7 |
| IgG2 | 10.0 |
| IgG3 | 0.05 |
| IgG4 | 0.2 |
| IgA | 0.7 |

N=4 assays

Precision (%CV)

Intra-assay precision is generated from the mean of the %CV's from four reportable results across 1 concentration of analytes in 4 different assays. Inter-assay precision is generated from the mean of the %CV's from four reportable results across 1 concentration of analytes across 4 different assays.

| Analyte | Intra-Assay (%CV) | Inter-Assay (%CV) |
|----------------|------------------------------|------------------------------|
| IgM | <11 | <15 |
| IgG1 | <11 | <15 |
| IgG3 | <11 | <15 |
| IgG4 | <11 | <15 |
| IgG2 | <11 | <15 |
| IgA | <11 | <15 |

Accuracy (% Recovery)

Spike Recovery: The data represent mean percent recovery of 4 levels of spiked standards in diluted serum from 4 different human samples.

| <i>Isotype</i> | <i>Spike Recovery in Serum</i> |
|-----------------------|---|
| IgM | 96 |
| IgG1 | 94 |
| IgG3 | 94 |
| IgG4 | 91 |
| IgG2 | 94 |
| IgA | 101 |

TROUBLESHOOTING GUIDE

| Situation | Possible Problem | Solution |
|--|--|--|
| Data acquisition time exceeds 30 seconds per well and/or "Sample Empty" occurs | <p><u>Mechanical</u></p> <ol style="list-style-type: none"> 1. Needle height is not correct (common problem due to variation in well depth between plate types). 2. Sample needle is clogged. 3. Air in the system. 4. Low pressure in the system. <p><u>Sample Related</u></p> <ol style="list-style-type: none"> 1. Lysate concentration too high. 2. Particulate matter in lysate. 3. No buffer in well. | <p><u>Mechanical</u></p> <ol style="list-style-type: none"> 1. Adjust needle height using 2 disks using "options; XY setup function". 2. Remove needle (see user's manual) and sonicate it to remove obstruction. 3. Perform alcohol flush and then wash with alcohol; followed by a wash with sheath fluid and a prime. 4. <u>Tighten</u> tops on the sheath fluid container. 5. <u>Loosen</u> the top on the waste container. <p><u>Sample Related</u></p> <ol style="list-style-type: none"> 1. Refer to lysate preparation protocol. 2. Centrifuge or filter lysate to remove particulate matter. |
| Readings are lower than expected | <ol style="list-style-type: none"> 1. Gate is not set properly. 2. Calibration is not correct. 3. Cells responded poorly to stimulation. | <ol style="list-style-type: none"> 1. Right click within the "doublet discriminator" and create gate. Move lines to 8,000 and 13,500 2. Run a machine calibration with calibration beads available from Luminex® Corp. 3. Check stimulation conditions. |

| | | |
|---|---|--|
| Bead pattern is diffuse and missing the bead target (white oval) | <ol style="list-style-type: none"> 1. Precipitate buildup in system. 2. Calibration is not correct. 3. Incompatible buffer used to resuspend beads for Luminex[®] analysis. | <ol style="list-style-type: none"> 1. Drain the system, followed by a backflush, proceed with solution for air in the system. 2. Run a machine calibration with calibration beads available from Luminex[®] Corp. 3. Vacuum plate and resuspend beads in Sheath Fluid. |
| Applying vacuum to filter plate does not remove liquid from wells | <ol style="list-style-type: none"> 1. Wells not in use are empty. 2. Particulate matter in lysate. | <ol style="list-style-type: none"> 1. Place tape over the top of empty wells that are not in use. 2. Pre-filter lysate before use. |
| Aggregation of beads during analysis | <ol style="list-style-type: none"> 1. Particulate matter in lysate. 2. Incompatible lysis buffer. 3. Beads not sonicated for step 3 of main protocol. | <ol style="list-style-type: none"> 1. Pre-filter the lysate. 2. Use recommended lysis buffer. 3. Sonicate resuspended 1X beads prior to adding to filter plate. |
| Liquid wicking out from 96-well filter plate | <ol style="list-style-type: none"> 1. Plate was not blotted on paper towel prior to adding next reagent. 2. The bottom of the plate is in contact with absorbent material such as paper towel or bench paper. | <ol style="list-style-type: none"> 1. After vacuum step, gently blot the bottom of the plate using a paper towel to remove excess liquid. 2. Place the plate on a flat, non-absorbent surface during loading steps. |

REPLACEMENT REAGENTS

Anti-Human Multi-Ig Beads, 1X
Anti-Human κ and λ Light Chain, PE
Human Multi-Immunoglobulin Standard
Human Immunoglobulin Positive Control
Assay Buffer
96-Well Filter Plate with 2 Sealers

Cat#

HGAM-PMX6
HGAM-1301
HGAM-8301
PC-301
L-AB
MX-PLATE

ORDERING INFORMATION

To place an order:

To assure the clarity of your kit order, please FAX the following information to our customer service department:

- Your name, telephone and/or fax number
- Customer account number
- Shipping and billing address
- Purchase order number
- Catalog number and description of product
- Quantity of kits

FAX: (636) 441-8050

Toll-Free US: (866) 441-8400
(636) 441-8400

Mail Orders: Millipore Corp.
6 Research Park Drive
St. Charles, Missouri 63304 U.S.A.

For International Customers:

To best serve our international customers in placing an order or obtaining additional information about MILLIPLEX MAP products, please contact your multiplex specialist or sales representative or email our European Customer Service at customerserviceEU@Millipore.com.

Conditions of Sale

All products are for research use only. They are not intended for use in clinical diagnosis or for administration to humans or animals. All products are intended for *in vitro* use only.

Material Safety Data Sheets (MSDS)

Material Safety Data Sheets for Millipore products may be ordered by fax or phone or through our website at www.millipore.com/techlibrary/index.do

WELL MAP

| | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | 10 | 11 | 12 |
|---|-----------------------------|---------------|----------------|---|---|---|---|---|---|----|----|----|
| A | Standard 0 Background | Standard 4 | Pos Control | | | | | | | | | |
| B | Standard 0 Background | Standard 4 | Pos Control | | | | | | | | | |
| C | Standard 1 | Standard 5 | | | | | | | | | | |
| D | Standard 1 | Standard 5 | | | | | | | | | | |
| E | Standard 2 | Standard 6 | | | | | | | | | | |
| F | Standard 2 | Standard 6 | | | | | | | | | | |
| G | Standard 3 | Standard 7 | | | | | | | | | | |
| H | Standard 3 | Standard 7 | | | | | | | | | | |